



ISSN: 2347-6567

International Journal of Allied Medical Sciences and Clinical Research (IJAMSCR)

IJAMSCR | Vol.14 | Issue 3 | July- Sep- 2026

www.ijamscr.com

DOI : <https://doi.org/10.61096/ijamscr.v14.iss3.2026.1239-1251>

Simultaneous Estimation of Niacin and Lovastatin by Using Rp-Hplc in Api and Marketed Formulations

T. Mahendhar*¹, Dr B Rajkamal, G. Devika, J. Venish, K. Vijay Krishna, K. Prathap

¹Department of Pharmaceutical Analysis, Avanthi Institute of Pharmaceutical Science, Gunthapally, Abdullapurmet, Near Ramoji Film City, Ranga Reddy, Telangana-501512.

Corresponding Author: T. Mahendhar

Email Id: principalgn@gmail.com



Published on:

15.07.2026

Published by:

Futuristic

Publications

2026 | All rights

reserved.



Creative Commons

Attribution 4.0

International

License.

Abstract: A novel, precise, accurate, rapid and cost effective isocratic reverse phase high performance liquid chromatographic (RP-HPLC) method was developed, optimized and validated for the estimation of Niacin and Lovastatin in bulk and pharmaceutical dosage forms. The drugs were estimated using Phenomenex Gemini C18 (4.6mm×150mm, 5µm) particle size column. A mobile phase composed of tri ethylamine buffer and methanol in proportion of 32:68 v/v, at a flow rate of 1.0 ml/min was used for the separation. Detection was carried out at 248nm. The linearity range obtained was 30-70µg/ml for Niacin and 10-50µg/ml for Lovastatin with retention times (Rt) of 3.297min and 5.405min for Niacin and Lovastatin respectively. The correlation coefficient values were found to be 0.999 & 0.999. Precision studies showed % RSD values less than 2 % for both the drugs in all the selected concentrations. The percentage recoveries of Niacin and Lovastatin were found to be 100.1873% for Niacin and 100.748% for Lovastatin respectively. The assay results of Niacin and Lovastatin were found to be 99.82%. The limit of detection (LOD) and limit of quantification (LOQ) were 2.6µg/ml and 7.8µg/ml for Niacin and 3.4µg/ml 10.2µg/ml for Lovastatin respectively. The proposed method was validated as per the International Conference on Harmonization (ICH) guidelines. The proposed validated method was successfully used for the quantitative analysis of commercially available dosage form.

Keywords: Niacin and Lovastatin, RP-HPLC, ICH Guidelines, Validation.

INTRODUCTION

Analytical chemistry is the branch of chemistry involved in separating, identifying and determining the relative amounts of the components making up a sample of matter. It is mainly involved in the qualitative identification or detection of compounds and the quantitative measurement of the substances present in bulk and pharmaceutical preparation.

Measurements of physical properties of analytes such as conductivity, electrode potential, light absorption or emission, mass to charge ratio, and fluorescence, began to be used for quantitative analysis of variety of inorganic and biochemical analytes. Highly efficient chromatographic and electrophoretic techniques began to replace distillation, extraction and precipitation for the separation of components of complex mixtures prior to their qualitative or quantitative determination. These newer methods for separating and determining chemical species are known collectively as instrumental methods of analysis. Most of the instrumental methods fit into one of the three following categories viz spectroscopy, electrochemistry and chromatography

Advantages of instrumental methods

- Small samples can be used

- High sensitivity is obtained
- Measurements obtained are reliable
- Determination is very fast
- Even complex samples can be handled easily

Limitations of instrumental methods

- An initial or continuous calibration is required
- Sensitivity and accuracy depends on the instrument
- Cost of equipment is large
- Concentration range is limited
- Specialized training is needed
- Sizable space is required

High Performance Liquid Chromatography

HPLC is a type of liquid chromatography that employs a liquid mobile phase and a very finely divided stationary phase. In order to obtain satisfactory flow rate liquid must be pressurized to a few thousands of pounds per square inch.

The rate of distribution of drugs between Stationary and mobile phase is controlled by diffusion process. If diffusion is minimized faster and effective separation can be achieved. The techniques of high performance liquid chromatography are so called because of its improved performance when compared to classical column chromatography advances in column chromatography into high speed, efficient, accurate and highly resolved method of separation.

For the recent study metformin and Sitagliptin was selected for estimation of amount of analyte present in formulation and bulk drug. The HPLC method is selected in the field of analytical chemistry, since this method is specific, robust, linear, precise and accurate and the limit of detection is low and also it offers the following advantages

- Speed many analysis can be accomplished in 20min (or) less.
- Greater sensitivity (various detectors can be employed).
- Improved resolution (wide variety of stationary phases).
- Re usable columns (expensive columns but can be used for many analysis).
- Ideal for the substances of low viscosity.
- Easy sample recovery, handling and maintenance.
- Instrumentation leads itself to automation and quantification (less time and less labour).
- Precise and reproducible.
- Integrator itself does calculations.
- Suitable for preparative liquid chromatography on a much larger scale.

EXPERIMENTAL METHODS

INSTRUMENTS USED

HPLC detector.	WATERS Alliance 2695 separation module, Software: Empower 2, 996 PDA
pH meter	Lab India
Weighing machine	Sartorius
Volumetric flasks	Borosil
Pipettes and Burettes	Borosil
Beakers	Borosil
Digital ultra sonicator	Lab man

CHEMICALS USED:

Niacin (Pure)	Sura labs
---------------	-----------

Lovastatin (Pure)	Sura labs
Water and Methanol for HPLC	LICHROSOLV (MERCK)
Acetonitrile for HPLC	Merck

HPLC METHOD DEVELOPMENT:

TRAILS

Preparation of standard solution:

Accurately weigh and transfer 10 mg of Niacin and Lovastatin working standard into a 10ml of clean dry volumetric flasks add about 7ml of Methanol and sonicate to dissolve and removal of air completely and make volume up to the mark with the same Methanol.

Further pipette 2.25ml of the above Niacin and 0.45ml of the Lovastatin stock solutions into a 10ml volumetric flask and dilute up to the mark with Methanol.

Procedure:

Inject the samples by changing the chromatographic conditions and record the chromatograms, note the conditions of proper peak elution for performing validation parameters as per ICH guidelines.

Mobile Phase Optimization:

Initially the mobile phase tried was Methanol: Water, Acetonitrile: Water with varying proportions. Finally, the mobile phase was optimized to Methanol: TEA buffer pH 4.8 in proportion 32:68 v/v respectively.

Optimization of Column:

The method was performed with various columns like C18 column, X- bridge column, Xterra. Phenomenex Gemini C18 (4.6mm×150mm, 5.0 µm) particle size was found to be ideal as it gave good peak shape and resolution at 1ml/min flow.

OPTIMIZED CHROMATOGRAPHIC CONDITIONS:

Instrument used	: Waters HPLC with auto sampler and PDA Detector 996 model.
Column	: Phenomenex Gemini C18 (4.6mm×150mm, 5.0 µm) particle size
Column temperature	: 38°C
pH	: 4.8
Mobile phase	: Methanol: TEA buffer pH 4.8 (32:68v/v)
Flow rate	: 1ml/min
Wavelength	: 248nm
Injection volume	: 20µl
Run time	: 7 min

METHOD VALIDATION

PREPARATION OF MOBILE PHASE:

Preparation of mobile phase:

Accurately measured 320ml (32%) of HPLC Methanol and 680ml of TEA buffer (68%) were mixed and degassed in a digital ultra sonicator for 15 minutes and then filtered through 0.45 µ filter under vacuum filtration.

Diluent Preparation:

The Mobile phase was used as the diluent.

RESULTS AND DISCUSSION

Trail 5 (Optimized Chromatogram):

Column	: Phenomenex Gemini C18 (4.6mm×150mm, 5.0 µm) particle size
Column temperature	: 38°C

Wavelength : 248nm
 Mobile phase ratio : Methanol: TEA buffer pH 4.8 (32:68v/v)
 Flow rate : 1ml/min
 Injection volume : 20µl
 Run time : 7 minutes

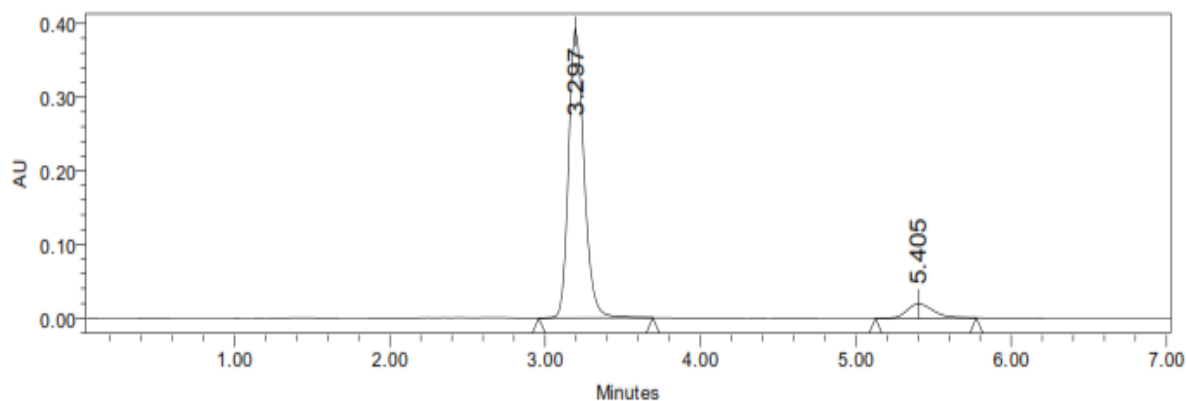


Figure: Optimized Chromatogram (Standard)

Table: Optimized Chromatogram (Standard)

S.No	Name	RT	Area	Height	USP Tailing	USP Plate Count	USP Resolution
1	Niacin	3.297	859856	42569	1.24	7896	
2	Lovastatin	5.405	5698	3652	1.36	6582	6.8

Observation: From the above chromatogram it was observed that the Niacin and Lovastatin peaks are well separated and they shows proper retention time, resolution, peak tail and plate count. So it's optimized trial.

Optimized Chromatogram (Sample)

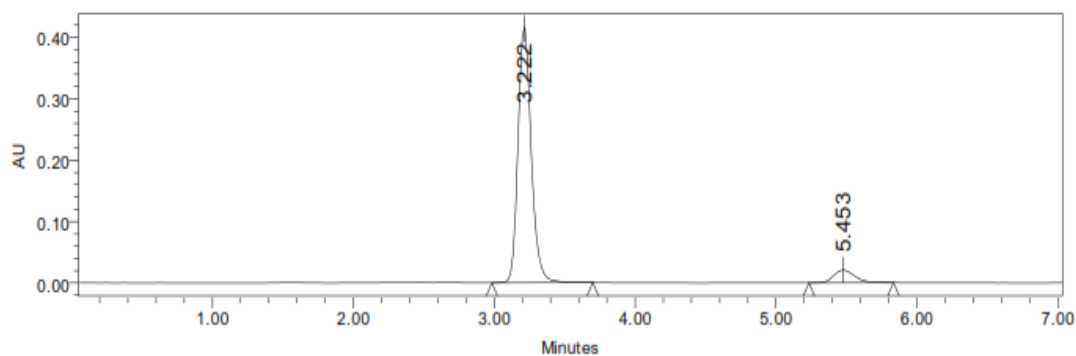


Figure: Optimized Chromatogram (Sample)

Table: Optimized Chromatogram (Sample)

No	Name	RT	Area	Height	USP Tailing	USP Plate Count	USP Resolution
1	Niacin	3.222	865898	43659	1.26	7985	
2	Lovastatin	5.453	5789	3785	1.38	6659	7.0

Acceptance Criteria:

- Resolution between two drugs must be not less than 2.
- Theoretical plates must be not less than 2000.
- Tailing factor must be not less than 0.9 and not more than 2.

- It was found from above data that all the system suitability parameters for developed method were within the limit.

METHOD VALIDATION

Blank:

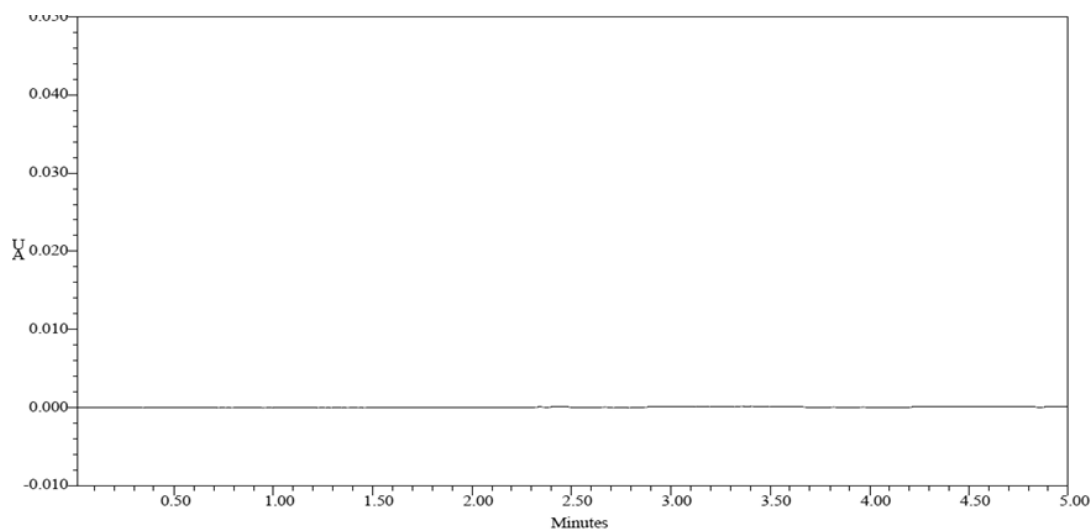


Fig: Chromatogram showing blank (mobile phase preparation)

System Suitability:

Table: Results of system Suitability for Niacin

S.No.	Peak Name	RT	Area ($\mu\text{V}\cdot\text{sec}$)	Height (μV)	USP Plate Count	USP Tailing
1	Niacin	3.200	859865	42568	7895	1.24
2	Niacin	3.248	859788	42587	7859	1.24
3	Niacin	3.299	857984	42659	7869	1.24
4	Niacin	3.297	854879	42875	7849	1.24
5	Niacin	3.297	857896	42487	7859	1.23
Mean			858082.4			
Std. Dev.			2024.409			
% RSD			0.235922			

Acceptance Criteria:

- %RSD of five different sample solutions should not more than 2.
- The %RSD obtained is within the limit, hence the method is suitable.

Table: Results of System Suitability for Lovastatin

S.No	Peak Name	RT	Area ($\mu\text{V}\cdot\text{sec}$)	Height (μV)	USP Plate Count	USP Tailing
1	Lovastatin	5.413	5689	3659	6583	1.36
2	Lovastatin	5.484	5687	3648	6592	1.37
3	Lovastatin	5.405	5682	3698	6549	1.37
4	Lovastatin	5.405	5649	3675	6571	1.36
5	Lovastatin	5.409	5674	3649	6529	1.36
Mean			5676.2			

Std. Dev.			16.2696			
% RSD			0.286628			

Acceptance Criteria:

- %RSD of five different sample solutions should not more than 2.
- The %RSD obtained is within the limit, hence the method is suitable.

SPECIFICITY

The ICH documents define specificity as the ability to assess unequivocally the analyte in the presence of components that may be expected to be present, such as impurities, degradation products, and matrix components.

Analytical method was tested for specificity to measure accurately quantitate Niacin and Lovastatin in drug product.

Assay (Standard):**Table: Peak Results for Assay Standard****Netupitant**

S.No.	Name	RT	Area	Height	USP Tailing	USP Plate Count
1	Niacin	3.211	859785	42598	1.25	7856
2	Niacin	3.222	859865	42895	1.24	7859
3	Niacin	3.254	857849	42578	1.25	7869

Palonosetron

S.No	Name	RT	Area	Height	USP Tailing	USP Plate Count	Resolution
1	Lovastatin	5.414	5699	3685	1.36	6598	6.9
2	Lovastatin	5.453	5687	3659	1.37	6537	6.9
3	Lovastatin	5.424	5689	3649	1.36	6582	7.0

Assay (Sample):**Table: Peak Results for Assay sample****Netupitant**

S.No	Name	RT	Area	Height	USP Tailing	USP Plate Count
1	Niacin	3.297	865985	43659	1.26	7985
2	Niacin	3.294	865798	43875	1.26	7925
3	Niacin	3.295	865456	43659	1.27	7946

Palonosetron

S.No	Name	RT	Area	Height	USP Tailing	USP Plate Count	Resolution
1	Lovastatin	5.435	5789	3659	1.37	6659	6.9
2	Lovastatin	5.417	5798	3684	1.38	6689	7.0
3	Lovastatin	5.434	5749	3695	1.38	6648	6.9

%ASSAY =

$$\frac{\text{Sample area}}{\text{Standard area}} \times \frac{\text{Weight of standard}}{\text{Dilution of standard}} \times \frac{\text{Dilution of standard}}{\text{Weight of standard}} \times \frac{\text{Purity}}{100} \times \frac{\text{Weight of tablet}}{\text{Label claim}} \times 100$$

The % purity of Niacin and Lovastatin in pharmaceutical dosage form was found to be 99.82%.

LINEARITY

CHROMATOGRAPHIC DATA FOR LINEARITY STUDY:

Niacin

Concentration $\mu\text{g/ml}$	Average Peak Area
30	545894
40	725985
50	897856
60	1068594
70	1245698

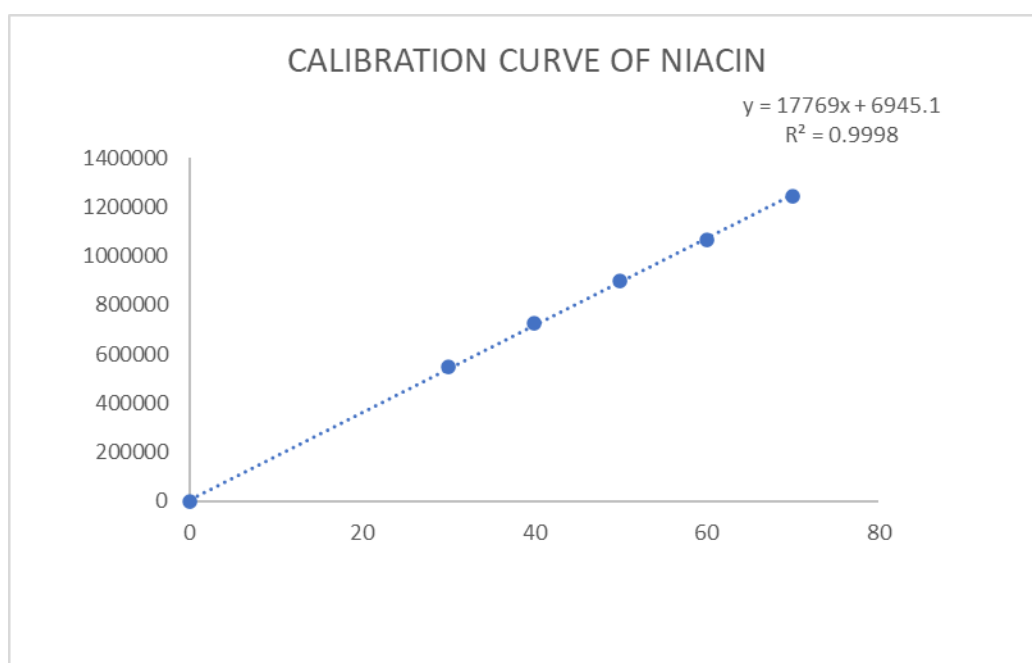


Fig: Calibration Curve of Niacin

LINEARITY PLOT:

The plot of Concentration (x) versus the Average Peak Area (y) data of Niacin is a straight line.

$$Y = mx + c$$

$$\text{Slope (m)} = 17769$$

$$\text{Intercept (c)} = 6945$$

$$\text{Correlation Coefficient (r)} = 0.999$$

VALIDATION CRITERIA: The response linearity is verified if the Correlation Coefficient is 0.99 or greater.

CONCLUSION: Correlation Coefficient (r) is 0.99, and the intercept is 6945. These values meet the validation criteria.

Palonosetron

Concentration $\mu\text{g/ml}$	Average Peak Area
10	2038

20	3859
30	5698
40	7489
50	9218

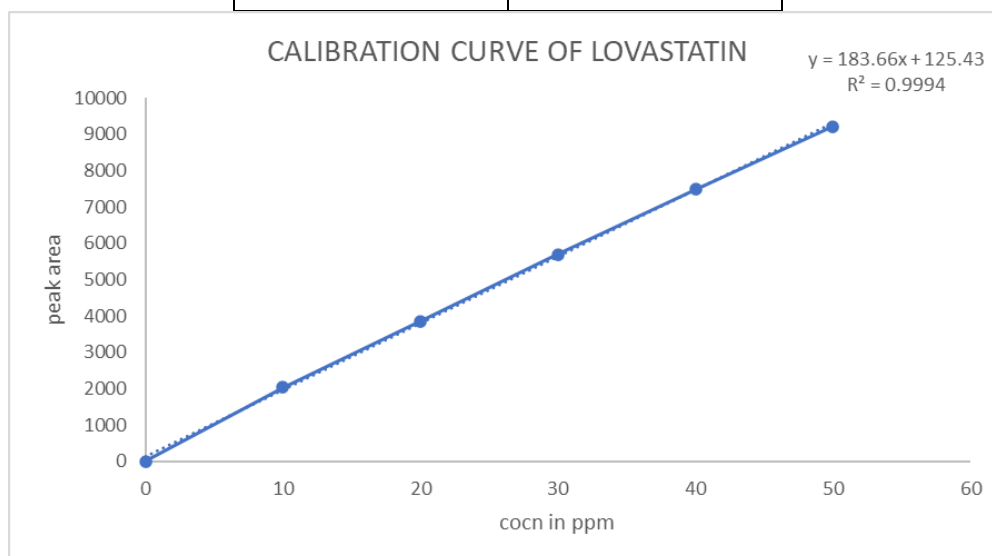


Fig: Calibration Curve of Lovastatin

LINEARITY PLOT:

The plot of Concentration (x) versus the Average Peak Area (y) data of Lovastatin is a straight line.

$$Y = mx + c$$

$$\text{Slope (m)} = 183.6$$

$$\text{Intercept (c)} = 125.4$$

$$\text{Correlation Coefficient (r)} = 0.999$$

VALIDATION CRITERIA: The response linearity is verified if the Correlation Coefficient is 0.99 or greater.

CONCLUSION: Correlation Coefficient (r) is 0.99, and the intercept is 125.4. These values meet the validation criteria.

PRECISION:

The precision of an analytical procedure expresses the closeness of agreement (degree of scatter) between a series of measurements obtained from multiple sampling of the same homogeneous sample under the prescribed conditions.

REPEATABILITY

Obtained Five (5) replicates of 100% accuracy solution as per experimental conditions. Recorded the peak areas and calculated % RSD.

Table: Results of Repeatability for Niacin:

S. No.	Peak name	Retention time	Area($\mu\text{V} \cdot \text{sec}$)	Height (μV)	USP Plate Count	USP Tailing
1	Niacin	3.213	859856	42659	7859	1.24
2	Niacin	3.253	857985	42598	7869	1.24
3	Niacin	3.297	856984	42587	7846	1.25
4	Niacin	3.215	856987	42569	7819	1.25

5	Niacin	3.254	859878	42894	7856	1.24
Mean			858338			
Std.dev			1454.222			
%RSD			0.169423			

Acceptance criteria:

- %RSD for sample should be NMT 2
- The %RSD for the standard solution is below 1, which is within the limits hence method is precise.

Table: Results of repeatability for Lovastatin :

S. No.	Peak Name	Retention time	Area ($\mu\text{V}\cdot\text{sec}$)	Height (μV)	USP Plate Count	USP Tailing
1	Lovastatin	5.441	5697	3659	6592	1.36
2	Lovastatin	5.442	5689	3648	6539	1.36
3	Lovastatin	5.409	5698	3692	6584	1.37
4	Lovastatin	5.520	5639	3648	6579	1.36
5	Lovastatin	5.424	5688	3689	6549	1.36
Mean			5682.2			
Std.dev			24.57031			
%RSD			0.432408			

Intermediate precision:**Day 1:****Table:** Results of Intermediate precision for Niacin

S.No.	Peak Name	RT	Area ($\mu\text{V}\cdot\text{sec}$)	Height (μV)	USP Plate count	USP Tailing
1	Niacin	3.211	868956	43659	7985	1.26
2	Niacin	3.211	869857	43985	7954	1.27
3	Niacin	3.210	865983	43879	7946	1.26
4	Niacin	3.212	866587	43865	7963	1.27
5	Niacin	3.211	864256	43875	7964	1.26
6	Niacin	3.297	868974	43562	7942	1.26
Mean			867435.5			
Std. Dev.			2167.095			
% RSD			0.249828			

Acceptance criteria:

- %RSD of six different sample solutions should not more than 2.

Table: Results of Intermediate precision for Lovastatin

S.No.	Peak Name	RT	Area ($\mu\text{V}\cdot\text{sec}$)	Height (μV)	USP Plate count	USP Tailing
1	Lovastatin	5.411	5785	3789	6659	1.37
2	Lovastatin	5.410	5798	3758	6625	1.38
3	Lovastatin	5.420	5766	3746	6649	1.38
4	Lovastatin	5.423	5746	3795	6675	1.37

5	Lovastatin	5.419	5782	3761	6653	1.38
6	Lovastatin	5.409	5786	3752	6627	1.37
Mean			5777.167			
Std. Dev.			18.40018			
% RSD			0.318498			

Acceptance Criteria:

- %RSD of six different sample solutions should not more than 2.

Day 2:**Table:** Results of Intermediate precision Day 2 for Niacin

S.No.	Peak Name	RT	Area (μV*sec)	Height (μV)	USPPlate Count	USPTailing
1	Niacin	3.211	845985	44585	8025	1.27
2	Niacin	3.233	847895	44895	8069	1.28
3	Niacin	3.244	848985	44758	8046	1.27
4	Niacin	3.297	847859	44548	8094	1.28
5	Niacin	3.297	845984	44865	8042	1.28
6	Niacin	3.202	847898	44254	8076	1.27
Mean			847434.3			
Std. Dev.			1201.345			
% RSD			0.141763			

Acceptance Criteria:

- %RSD of six different sample solutions should not more than 2.

Table: Results of Intermediate precision Day 2 for Lovastatin

S.No.	Peak Name	RT	Area (μV*sec)	Height (μV)	USPPlate Count	USPTailing
1	Lovastatin	5.411	5898	3986	6852	1.39
2	Lovastatin	5.410	5884	3955	6864	1.39
3	Lovastatin	5.420	5863	3956	6829	1.40
4	Lovastatin	5.405	5845	3945	6874	1.39
5	Lovastatin	5.409	5896	3925	6829	1.39
6	Lovastatin	5.463	5874	3962	6825	1.40
Mean			5876.667			
Std. Dev.			20.39281			
% RSD			0.347013			

Acceptance Criteria:

- %RSD of six different sample solutions should not more than 2.

ACCURACY:

Accuracy at different concentrations (50%, 100%, and 150%) was prepared and the % recovery was calculated.

Table: The accuracy results for Niacin

% Concentration (at specification Level)	Area	Amount Added (ppm)	Amount Found (ppm)	% Recovery	Mean Recovery
50%	451144.3	25	24.998	99.992%	100.1873%

100%	897248.3	50	50.104	100.208%	
150%	1344562	75	75.278	100.362%	

Acceptance Criteria:

- The percentage recovery was found to be within the limit (98-102%).

The results obtained for recovery at 50%, 100%, 150% are within the limits. Hence method is accurate.

Table : The accuracy Results for Lovastatin

%Concentration (at specification Level)	Area	Amount Added (ppm)	Amount Found (ppm)	% Recovery	Mean Recovery
50%	2895	15	15.084	100.560%	100.748%
100%	5685.333	30	30.282	100.940%	
150%	8449	45	45.335	100.744%	

Acceptance Criteria:

- The percentage recovery was found to be within the limit (98-102%).

The results obtained for recovery at 50%, 100%, 150% are within the limits. Hence method is accurate.

LIMIT OF DETECTION

The detection limit of an individual analytical procedure is the lowest amount of analyte in a sample which can be detected but not necessarily quantitated as an exact value.

$$LOD = 3.3 \times \sigma / s$$

Where

σ = Standard deviation of the response

S = Slope of the calibration curve

Niacin:

Result: =2.6 μ g/ml

Lovastatin:

Result: =3.4 μ g/ml

Quantitation limit

The quantitation limit of an individual analytical procedure is the lowest amount of analyte in a sample which can be quantitatively determined.

$$LOQ = 10 \times \sigma / S$$

Where

σ = Standard deviation of the response

S = Slope of the calibration curve

Niacin:

Result: =7.8 μ g/ml

Lovastatin:

Result: =10.2 μ g/ml

ROBUSTNESS

The robustness was performed for the flow rate variations from 0.9 ml/min to 1.1ml/min and mobile phase ratio variation from more organic phase to less organic phase ratio for Niacin & Lovastatin. The method is robust only in less flow condition and the method is robust even by change in the Mobile phase $\pm 5\%$. The standard sample of Niacin & Lovastatin were injected by changing the conditions of chromatography. There was no significant change in the parameters like resolution, tailing factor and plate count.

Variation in flow

Table: Results for Robustness**Niacin:**

Parameter used for sample analysis	Peak Area	Retention Time	Theoretical plates	Tailing factor
Actual Flow rate of 1.0mL/min	859856	3.297	7896	1.24
Less Flow rate of 0.9mL/min	915847	3.639	7251	1.20
More Flow rate of 1.1mL/min	842564	2.859	7415	1.21
Less organic phase (about 5 % decrease in organic phase)	825498	3.460	7365	1.23
More organic phase (about 5 % Increase in organic phase)	814578	3.022	7258	1.22

Acceptance Criteria:

The tailing factor should be less than 2.0 and the number of theoretical plates (N) should be more than 2000.

Table: Results for Robustness**Lovastatin:**

Parameter used for sample analysis	Peak Area	Retention Time	Theoretical plates	Tailing factor
Actual Flow rate of 1.1mL/min	5698	5.405	6582	1.36
Less Flow rate of 0.9mL/min	6452	6.250	6785	1.32
More Flow rate of 0.8mL/min	5254	4.863	6365	1.34
Less organic phase (about 5 % decrease in organic phase)	5487	6.196	6254	1.38
More organic phase (about 5 % Increase in organic phase)	5369	5.010	6298	1.33

Acceptance Criteria:

The tailing factor should be less than 2.0 and the number of theoretical plates (N) should be more than 2000.

SUMMARY AND CONCLUSION

High performance liquid chromatography is at present one of the most sophisticated tool of the analysis. The estimation of Niacin and Lovastatin was done by RP-HPLC.

The TEA buffer was p^H 4.8 and the mobile phase was optimized with consists of Methanol: TEA buffer mixed in the ratio of 32:68 % v/v.

A Phenomenex Gemini C18 (4.6mm×150mm, 5.0 μ m) particle size or equivalent chemically bonded to porous silica particles was used as stationary phase.

The solutions were chromatographed at a constant flow rate of 1.0 ml/min. The linearity range of Niacin and Lovastatin were found to be from 30-70 μ g/ml, 10-50 μ g/ml respectively. Linear regression coefficient was not more than 0.999, 0.999.

The values of % RSD are less than 2% indicating accuracy and precision of the method. The percentage recovery varies from 98-102% of Niacin and Lovastatin. LOD and LOQ were found to be within limit.

The results obtained on the validation parameters met ICH and USP requirements. It inferred the method found to be simple, accurate, precise and linear.

The method was found to be having suitable application in routine laboratory analysis with high degree of accuracy and precision.

ACKNOWLEDGEMENT

The Authors are thankful to the Management and Principal, Avanthi Institute of Pharmaceutical Science, Gunthapally, Abdullapurmet, Telangana, for extending support to carry out the research work. Finally, the authors express their gratitude to the Sura Pharma Labs, Dilsukhnagar, Hyderabad, for providing research equipment and facilities.

REFERENCES

1. Meyer V.R. Practical High-Performance Liquid Chromatography, 4th Ed. England, John Wiley & Sons Ltd, (2004), PP 7-8.
2. Sahajwalla CG a new drug development, vol 141, Marcel Dekker Inc., New York, (2004), PP 421–426.
3. Introduction to Column. (Online),URL:http://amitpatel745.topcities.com/index_files/study/column_care.pdf
4. Detectors used in HPLC (online)URL:http://wiki.answers.com/Q/What_detectors_are_used_in_HPLC
5. Detectors (online) ,URL:http://hplc.chem.shu.edu/NEW/HPLC_Book/Detectors/det_uvda.html
6. Dr.Kealey and P.J.Haines, Analytical Chemistry, 1st edition, Bios Publisher,(2002),PP:1-7.
7. A.BraithWait and F.J.Smith, Chromatographic Methods, 5th edition, Kluwer Academic Publisher, (1996), PP 1-2.
8. Andrea Weston and Phyllisr. Brown, HPLC Principle and Practice, 1st edition, Academic press, (1997), PP 24-37.
9. Yuri Kazakevich and Rosario Lobrutto, HPLC for Pharmaceutical Scientists, 1st edition, Wiley Interscience A JohnWiley & Sons, Inc., Publication, (2007), PP 15-23.
10. Chromatography, (online). URL:<http://en.wikipedia.org/wiki/Chromatography>.
11. Draft ICH Guidelines on Validation of Analytical Procedures Definitions and terminology. Federal Register, vol 60. IFPMA, Switzerland, (1995), PP 1126.
12. Code Q2B, Validation of Analytical Procedures; Methodology. ICH Harmonized Tripartite Guidelines, Geneva, Switzerland, (1996), PP 1- 8.
13. Introduction to analytical method validation (online), available from: URL: <http://www.standardbase.hu/tech/HPLC%20validation%20PE.pdf>.
14. Data elements required for assay validation, (online) available from: URL: <http://www.labcompliance.com/tutorial/methods/default.aspx>.
15. Snyder LR practical HPLC method development, 2nd edition. John Wiley and sons, New York, (1997), PP 180-182.
16. Skoog D A, West D M, Holler FJ: Introduction of analytical chemistry. Sounder college of publishing, Harcourt Brace college publishers. (1994), PP 1-5.
17. Sharma B K, Instrumental method of chemical analysis Meerut. (1999), PP 175-203.
18. Willard, H. y. Merritt L.L, Dean J.A and Settle F.A “Instrumental methods of analysis” 7th edition CBS publisher and distributors, New Delhi, (1991), PP 436-439.
19. ICH Q2A, “validation of analytical methods, definitions and terminology”, ICH Harmonized tripartite guideline, (1999).
20. <https://www.drugbank.ca/drugs/DB00627>